

GeneProof®

Brachyspira hyodysenteriae PCR Detection Kit



in vitro Diagnostics

The kit is designed for professional use in specialized clinical and research laboratories.

Method principles

This kit is designed for the genomic DNA detection in *Brachyspira hyodysenteriae* by the Polymerase Chain Reaction method (PCR). The detection is focused on the pF12 clone sequence specific for *Brachyspira hyodysenteriae*. The procedure takes an advantage of the "hot start" technology, minimizing non-specific reactions and assuring maximum sensitivity. The reaction mix includes an internal standard controlling the possible inhibition of the PCR reaction and the uracil-DNA-glycosylase (UDG) controlling possible contamination by amplification products. Sensitivity of this method is 10¹ copies of genomic DNA per reaction. DNA isolation recommended by means of commercial kits designed for nucleic acid isolation.

Kit composition

	Cat. No. BH/E/ISIN/025 25 reactions	Cat. No. BH/E/ISIN/050 50 reactions	Cat. No. BH/E/ISIN/100 100 reactions
MasterMix <i>Brachyspira hyodysenteriae</i>	1 x 900 µl	2 x 900 µl	4 x 900 µl
Positive control <i>Brachyspira hyodysenteriae</i> 10 ² copies/µl	1 x 50 µl	1 x 50 µl	2 x 50 µl

Storage and transportation conditions

Transport the kits at temperatures ranging from -20 °C to -80 °C. The kit remains stable for at least 6 months from the date of manufacturing at the temperature of -20 °C. Repeated freezing and thawing of the MasterMix and the Positive control may result in lower detection quality. The manufacturer therefore recommends to distribute the MasterMix by 36 µl directly to PCR tubes and hold in stock at -20 °C. Positive control may be held in stock at 4 °C.

User Manual

Sampling and sample storage

Sampling of all sample types should be performed into sterile tubes without any transportation media and the samples should be transported within 12 hours at +4 °C. It is necessary to sample up to 2 ml of body fluid samples or take wad smears or swabs "dry". In case of longer storage all samples should be frozen at -20 °C.

DNA isolation

Isolation recommended by means of commercial DNA isolation kits according to the particular protocols of the isolation kit manufacturers. The manufacturer recommends the following isolation kits: PathogenFree DNA isolation kit (GeneProof); QIAamp DNA Blood Mini Kit (QIAGEN); NucleoSpin Blood (Macherey-Nagel).

PCR amplification

1. Add 36 μ l of the MasterMix and 4 μ l of the DNA isolate or 4 μ l of the Positive control into the PCR tube. The final reaction mix volume should be 40 μ l.*
2. Insert the tubes into a thermocycler and amplify them according to the following recommended program:
Amplification program: **

UDG decontamination	37 °C/5 min.
initial denaturation	96 °C/15 min.
denaturation	96 °C/20 sec.
annealing	56 °C/20 sec.
extension	72 °C/40 sec.
number of cycles	45
final extension	72 °C/2 min.

*Tubes should be maintained in cold environment when handled (at 0 – 15 °C)

**Hereby presented amplification conditions may differ for various types of thermocyclers. The above listed conditions apply for PTC 200 (MJ Research) thermocycler.

Agarose electrophoresis

The resulting amplification products should be separated on 2% agarose gel electrophoresis (5V/cm) containing Ethidium bromide (5 μ g/1 ml) and visualized by means of UV illumination. Since the loading buffer is included in the reaction mix, there should be directly loaded at least 10 μ l of the amplification product.

Detection evaluation

Positive sample – is the detected amplification product with the length of 172 bp, there may also be the detected amplification product of the internal standard with the length of 591 bp (Fig. 1; track 4).

Negative sample – only the amplification product of the internal standard with the length of 591 bp is detected (Fig. 1; tracks 2-3).

Inhibiting sample - should inhibition of the reaction components occur or should the reaction fail to proceed, none of the above-listed amplification products would be detected and the examination should be repeated. (Fig. 1; track 1).

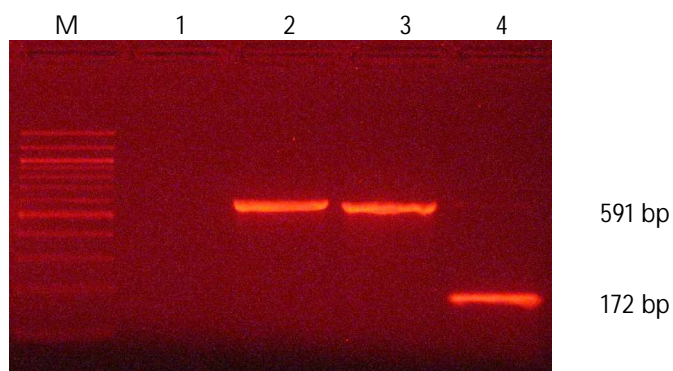


Fig. 1. Electrophoretical detection of amplification products on 2% agarose gel. M is a 100bp weight marker.

Warning:

- Ø Be very careful when handling the Positive control or the clinical material – incorrect handling could result in contamination and the consequent impairment of the kit components or the MasterMix! The manufacturer is not responsible for the kit impairment due to incorrect handling.
- Ø The kit should be disposed of after use according to the current legal regulations considering the fact that the kit doesn't contain any dangerous, infectious or toxic components that would be subject to special safety regulations and the packaging materials are made of paper and polypropylene.
- Ø Service fee assuring returnability and recycling of the waste packaging material has been paid under the identification number EK-F00041495.

Manufacturer: GeneProof a.s.
Viniční 235, Brno, Czech Republic
E-mail: info@geneproof.eu, Phone/Fax: +420 543 211 679

Issue Date: February 14, 2006

Last Revision Date: July 3, 2006